

CRYOPROBES CATALOGUE

CRYO-S® Mini


GYNECOLOGY



GYNECOLOGY


G-10/20/RF

REF. number	
0 4 1020 1	
Designed for	
Cryoprobe for cervix Ø 20 mm	
Up to 50 treatments	

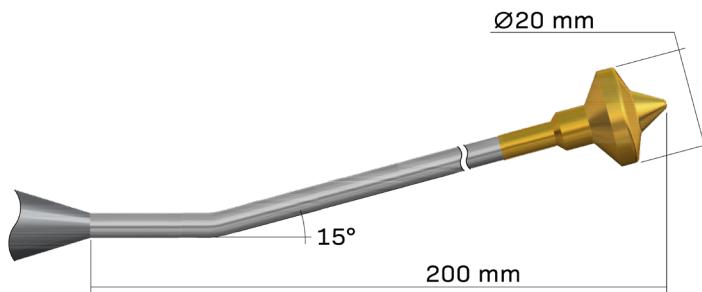

G-10/22/RF

Numer REF.	
0 4 1022 1	
Designed for	
Cryoprobe for cervix Ø 22 mm	
Up to 50 treatments	

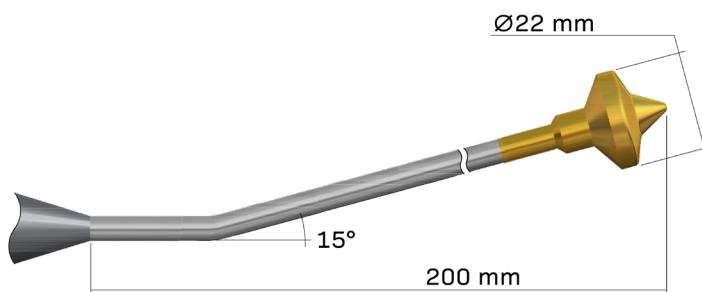


Expiration date of reusable cryoprobes is 6 years or until the max. number of treatments is reached

GYNECOLOGY


G-10/24/RF

REF. number	
0 4 1024 1	
Designed for	
Cryoprobe for cervix Ø 24 mm	
Up to 50 treatments	

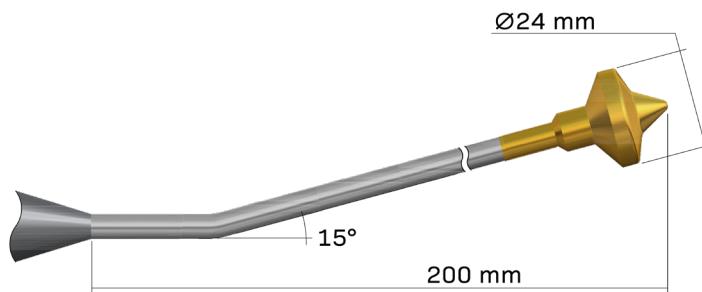

G-40/4/RF

REF. number	
0 4 4004 1	
Designed for	
Cryoprobe for endometrial ablation.	
Up to 50 treatments	

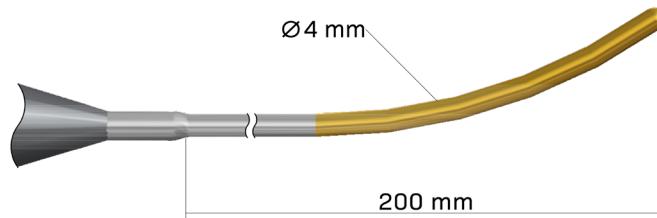


Expiration date of reusable cryoprobe is 6 years or until the max. number of treatments is reached

GYNECOLOGY

G-60/RF

REF. number	
0 4 6015 1	
Designed for	
Flat cryoprobe for cervix (nullgravidas).	


Up to 50 treatments

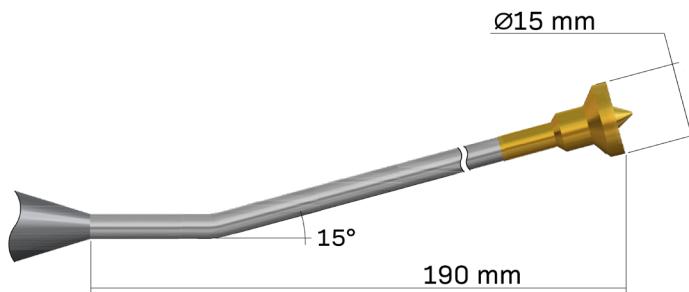

G-70/RF

REF. number	
0 4 7015 1	
Designed for	
Short cryoprobe for cervical canal	

Up to 50 treatments

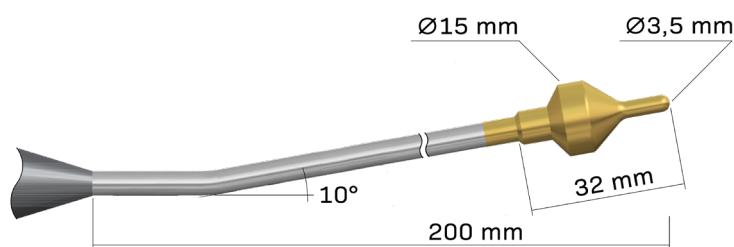

Expiration date of reusable cryoprobes is 6 years or until the max. number of treatments is reached



IND-2023-06-ELECTRIC-01-EN



METRUM CRYOFLEX Sp. z o.o.

Manufacture

ul. Zielna 29
05-082 Blizne Łaszczyńskiego
POLAND, EU

Headoffice

ul. Kolejowa 33
05-092 Łomianki
POLAND, EU

Tel.: +4822 33 13 750

+4822 33 13 830

export@metrum.com.pl
<https://www.metrum.com.pl>

In care for highest quality of offered products and services, METRUM CRYOFLEX reserves the right to modify products and introduce changes in descriptions.